Assembly station

versie 2new

Contents

1 Introduction **2**

2 Monitored Drift Tube Chambers **3**

2.1 Assembly of BOL-chambers at NIKHEF 3

3 Preparation of the Assembly Station **3**

3.1 The global and chamber coordinate system 4

3.2 The 'Frascati' combs 4

3.3 The Tube combs 5

3.4 The Sphere towers 5

3.5 Positionning of the mechanics on the table 5

3.6 Frascati comb positioning 5

3.7 Tube comb positioning 6

3.8 Sphere tower positioning 6

4 Machinery for Assembly and Gluing **7**

4.1 Sag Compensation 7

5 Assembly Monitoring **8**

5.1 RASAS system 8

5.1.1 Calibration Constants 9

5.2 RASNIK systems on the spacer 10

5.3 End-Plug Laser System 10

5.4 Automated assembly manager 11

6 Assembly Procedure **18**

6.1 Assembly of the bare spacer 18

6.2 The gluing of tube layers 18

7 Control of chamber assembly **20**

7.1 Control of the tube position 23

7.2 Layer-pitch control 23
7.2.1 Layer Z-pitch 23
7.2.2 Layer Y-pitch 24
7.3 Relative positioning at the middle cross-plate 24
7.4 Final measurements 24

8 Results of X-ray scans **25**

9 Further investigation and Additional Checks **26**
9.1 Tube layer pitch 26
9.2 Temperature Gradients 26

10 Conclusions **27**

A Measurement tools **27**
A.1 The Heigth-meter 27
A.2 The malmonitor 27
A.3 Laser optics 28
A.4 Silicon Sensor 28
A.5 Bol-monitor 28
A.6 Calibration tower for RASAS system 28
A.7 Calibration tower for In-Plane masks 29

1 Introduction

The task of the ATLAS detector at the LHC is to discover the Higgs boson and to be prepared for the unexpected, e.g. new physics. Both requirements are covered by a detector optimized for final state muons with high momentum.

New physics can lead to events with muons that emerge with a transverse momentum of 1 TeV. To be able to detect these interactions an accuracy of the order $\frac{\sigma_{P_T}}{P_T}$=10% is needed. This translates to 50 μm uncertainty on the sagitta measurement in the 2 Tm magnetic field, provided by an air core toroid. At these energies, the major contributions to this uncertainty originate from the detector alignment and the wire positions. Therefore, the accuracy of these contributions should not exceed the (about) 20 μm . At lower energies, 100 GeV, the momentum resolution is a few percent, dominated by energy loss fluctuations in the inner detector.

The barrel muon system measures three space points. Each point is measured by 6 drift tubes with an single hit resolution of about 100 μm . In some parts of the end-cap muon system the muon momentum has to be extraced from the also measured direction of the muon trajectory, leading to a slightly less accurate measurement.

In this report we describe the construction of the muon detector at NIKHEF, where the production of the outer layer of the barrel has commenced.

2 Monitored Drift Tube Chambers

Figure 3 shows a muon chambers consisting of two panels (multi-layers), each with three drift tube layers, separated by a support structure, the spacer. The spacer consists of three beams, called crossplates, that run orthogonal to the tubes which connect the multilayers. The crossplates are connected by two beams, called longbeams.

The drift tubes are the basic detection elements of the MDTs. These tubes have a diameter of $29.970^{+0.030}_{-0.000}$ mm and are closed by precise end-plug which center the 50 μm gold-plated tungsten wire. The wire is fixed under tension (about 280 gram) leading to a gravitational sag of about 400 μm for a tube with a length of 5 m. The intension is to adjust the sag of the chambers, depending on their orientation in ATLAS, such that the wires are centered with respect to the tubes with an RMS of 100 μm .

The end-plugs are manufactured with a precise outer ring that allows to position the tubes during the assemblyin jigs with high precision. A so called twister centers the wire.

Physical deformations of the chambers during construction, transport and operation are monitored with the In-Plane alignment system. This system consist logically of four RASNIK systems as shown in Fig. 3. In a test setup at CERN [**?**] an alignment accuracy better than 10 μm (on the wire position) can be achieved with this system. In addition, 14 temperature sensors deliver aanvullende information.

2.1 Assembly of BOL-chambers at NIKHEF

The task of NIKHEF is to assemble 96 'Barrel Outer Large' (BOL) chambers, which have dimensions of approximatley 5 m$\times$2 m, with a mechanical precision of 20 μm on the wire positions. Over the past two years the assembly station, based on a granite block, has been prepared. Figure 3 shows the assembly station. The jigs or 'combs' which position the tubes of a single tube-layer are visible. The assembly procedure starts with the assembly of the bare spacer to wich the tubes, layer by layer, are attached using glue. To avoid large deformations of the spacer due to the weigth of tube-layers, the layers are glued one by one on each side of the spacer. This involves, several times, rotating the spacer (and already attached tube-layers on it) during assembly, but avoids a large assymetric weight distribution.

In this report we present the preparation of the assembly station, the assembly of the first ten BOL chambers and the test of three BOL chambers in the tomograph at CERN.

3 Preparation of the Assembly Station

granite table with dimensions (l$\times$w$\times$h) 5.5 m$\times$2.5 m$\times$0.5 m forms the basis of the assembly station. A new tube-layer to be attached on the spacer (or on the spacer with some tube layers already attached to it) is position in jigs. The spacer is positioned by six sphere holders, and, supported by a sag compensation system. Figure 3 displays one precision tower. The removable 'ears' on the spacer accomodate a sphere that is support by the sphere holders on the towers. Figure 3 displays one precision tower, supporting the ear of the bare spacer. The towers can be adjusted in heigth by changing the 'stacking blocks' corresponding to thickness of tube layers that have been attached to the spacer, during the gluing process. Figure 3 also shows the alignment system, RASAS, that monitors the position of the ears.

3.1 The global and chamber coordinate system

The global coordinate system (at NIKHEF) is defined such that it coincides with the local chamber system, when the chamber is located on the granite table in the 'up' position. The Y coordinate points to the sky, the X coordinate lays in the horizontal plane and runs along the tubes, the long dimension of the chamber. The Z coordinate is the precision coordinate and runs perpendicular to the tubes. During assembly we flip the chamber to the 'down' position, by effectively rotating it over its Z axis.

In the cleanroom, we defined North and South as the $+X$ and $-X$ side respectively. In the 'up' ('down') position the RO and HV (HV and RO) side coincides with South and North respectively. The X, Y and Z axis form a left-handed system.

The so called 'reference-side' of the chamber is choosen to be the negative (or smallest) Z side and coincides with 'West'.

We follow the specs given in the ATLAS MUON TDR (page 138). Combining the intrinsic accuracy and the positioning accuracy we summarize:

- The Y, Z accuracy of Frascati-combs and towers has to be 10 μm .
- The X accuracy has a spec of 100 μm .
- Angles A_X, A_Y and A_Z of the Frascatie combs have to be precise to 25 μrad , 0.5 mrad and 0.5 mrad respectively.
- The concentricity of the wire in the tubes has to be accurate to 100 μm RMS.

We aim to align the combs and towers such that the wire positions in the bending plane are controlled within 20 μm . The wires are centered in the tubes over the full length of the tubes within 100 μm . Finally, we mention the importance of the torque, i.e., the angular difference between the North and South Frascati combs. The torque should be know whithin 20 μrad . In Appendix A, the tools used for the alignment of the assembly station are decribed in detail. Below we discuss the various elements of the assembly station and in particular their accuracy.

3.2 The 'Frascati' combs

The precision combs holding the tubeplugs at the HV and RO ends during the glueing of a tubelayer were assembled at Frascati. They consist of 4 aluminum pieces with glued steel precision rods to position the plugs. These pieces were produced using a master jig as descibed in [ref.Frascati], and then glued together to make one 72 tube BOL jig. The assembled combs were measured on a CNC machine at NIKHEF. The analysis of the measurements showed :

- the average z-pitch of the two complete combs is 35.0355mm at a temperature [1] 20.4 +- 0.4 ^{o}C and deviations of < 0.1 μm from this value for the average z-pitch of the original jig pieces.
- The rms of the individual z positions and the rms of the y-deviations from a straight line are less than 2 μm . No significant systematic shifts in z or y were found at the glue joints of the 4 pieces.

[1] The temperature was stable at the level of 0.1^{o}C during the measurements with the 3D coordinate measuring machine. However, we discovered inconsistencies on the absolute value of the temperature reading. Due to this problem we assign an uncertainty of 0.4^{o}C.

3.3 The Tube combs

The combs supporting the tubes inbetween the precision combs at 0.5m intervals ,have been machined at NIKHEF as solid aluminum pieces with a width corresponding to 18 tubes.A total of 50 pieces were produced en measured on the CNC.

To assemble the 9 full width combs (72 tubes) the 36 best pieces were selected, taking into account the precision of the wedges and the connecting surfaces. The connections between the pieces were checked with the RASNIK malmonitor device prior to their fixation.

The assembled combs were again measured on the CNC and the results were compared with the nominal height and Frascati pitch. The RMS deviations of the tube positions are less than 15 μm in z and y.

3.4 The Sphere towers

The sphere towers consist of a base block, one of 3 different type of stacking blocks to adjust the spacer position according to the type of layer to be glued, and a top block with the sphere holder.

Measurements with the CNC machine of all the separate parts allowed a selection of optimal combinations of base, stacking and holder blocks resulting in a Y and Z accuracy of about 5 μm .

3.5 Positionning of the mechanics on the table

The accuracy of the Y position of the mechanics is limited by the flatness of the granite table. Over short distances (one meter) this accuracy is about 10 μm . Over longer distances, temperature gradients start to play a role, which make the table bend and can lead to a sagitta of 25 μm over five meter.

The combs and towers are initially positionned with low accuracy. The high precision is reached by adjustments and many remeasurements in an iterative way.

Both the precision and tube combs are positionned on the table with a sliding fixation such that they are allowed to expand freely in the direction away from the reference bar in case of temperature variations. This was checked with laser interferometer measurements and local heating of some combs with approximately +5 deg temperature increase.

3.6 Frascati comb positioning

In order to properly combine the Frascati combs with tube combs a 20 μm steel foil was used to shim the height of the Frascati combs on the assembly table. This was needed due to a small change in the tube and plug geometry after the combs were already machined.

The relative height above the table surface of the precision wedges was checked several times before and during chamber construction with heigth-meter measurements. Average deviations from the nominal value were found to be less than 5 μm with an rms below 4 μm for different positions along the combs.

The relative torque of the Frascati combs is measured by using tiltmeters. Despite the high intrinsic precision precison of these tiltmeters, a measurement better than than 10 μrad seems

impossible. We measured the torque to be zero whithin the scatter of the measurements.

The X distance was based on a test-TUBE with known length and rechecked by tape-measure. The X-distance between the tube supports is stable within 500 μm , dominated by the low precision of the X coordinate of these supports themselves.

To measure the angle (the parallelness) between the two Frascati combs, a laser beam in the X direction is used, aligned by the silicon sensor on the first wedges of the Frascati combs. A penta prism, accurate to 10 μrad , reflects the laserbeam over an angle of 90 degrees into the Z direction. The Frascati combs are aligned with respect to this beam, leading to a straigthness in X within 100 μm . Thus, seen in the X-Z plane, the Frascati combs describe a rectangular shape with angular deviations of about 100 μrad .

3.7 Tube comb positioning

The tube combs are positionned on the assembly table with one side fixed to a reference bar. Each jig position is adjusted in Z such that the tube positions of the 9 combs deviate less than 50 μm from straight lines connecting the two precision combs at each end of the table.

For this we used a laser and silicon-sensor combination (see A) The laser beam defines a straight line between the two precison combs roughly along path of a tube. The relative beam position in Z and Y is measured by the silicon sensor.

These measurements are repeated at several positions along the precision combs. In fig [sisens] we show the distribution of the deviations for some of the measurements. The rms of the deviations is typically xx μm in z and yy μm in y, thus amply fulfilling the requirement of 100 μm rms for the centrisity of the wire with respect to the tube centre. These measurements will be repeated regularly as part of the QA/QC procedure.

Heigth meter measurements directly comparing the relative height of corresponding wedges in the Frascati combs and in the tube combs next to them showed deviations less than 20 μm from the nominal value. This ensures that the alignment platforms which are glued onto the first tubelayer in this area can be positionned with with sufficient precision.

3.8 Sphere tower positioning

The sphere towers will support the spacer during the gluing procedure and so determine the wire positions between the several tube layers. The towers are initially positioned with an accuracy in the Z direction of about 100 μm using standard optical tools.

The alignement in Y of the three refence towers is checked with the silicon sensor. The results indicate that the middle tower with respect to a line defined by the Y of the outer towers deviates by -25 $\pm$ 10 μm . The non reference side is checked in a similar way, which reveals the same deviation. The intrinsic accuracy of these towers is does not allow such deviation, leading to the conclusion that the surface of the granite table, at the position of the towers, has deviations of the same order. We tried to find more evidence, but to measure with this accuracy over 5 m is far from trivial. However, (re)measurements with standard optical tools indeed suggest a negative deviation in heigth of the central towers.

On the reference side of the table the sphere towers are fixed to the corresponding Frascati combs. In order to assure that the two multilayers are glued to the spacer without a significant stereo angle between them, the distance between the wedges and the spacer fixation in z must differ by less

than 10 μm for the two precision combs. This is because the HV and RO ends of a chamber are interchanged with respect to the two precision combs for glueing either of the two multilayers (see 3.1). For the QA/QC of this requirement we use an auxiliary device called the BOL-monitor as describes in A.

An recent example of such a measurement is shown in fig [xyzbol11.ps]. Here we plot the difference in Z and Y position of the cross plate lenses with respect to the two precision combs, as measured on the North and South side of the assembly table. The position difference is plotted as function of the X position of the forks; X=0 corresponding to the lens being in the middle between the mask and the CCD of of the Rasnik system. The X values are derived from magnification of the mask image on the CCD. Straight lines are fit through the two corresponding sets of data at the North and South side respectively. The points show the deviations of the measurements on the North side from the line fit throught the measurements on the South side, and vice versa. The two colors differentiate between the two orientations of the monitor cross-plate, which in principle should lead to the same result. The corresponding lens positions are indicated by Reference side and NonReference side. For the DZ measurement the the Reference side data are the most reliable, as the distance between the reference tower and the lens is short (30 cm) and temperature effects can be neglected. For the Non-Ref Z measurements the lens is at 210 cm from the reference tower and its position is thus subject to temperature differences of the cross-plate and the combs between North and South data sets, which are not corrected for. For the DY measurements the temperature effects can be neglected .

From the plot one can see that with both orientations of the cross-plate we measure at the Ref side a difference in Z of 6 μm , which is within the 10 μm tolerance. This value has remained the same within $\pm$5 μm over 2 years since the comb positions were fixed.

The Y differences are much less critical for the chamber assembly, since the glueing procedure assures that the distance between the two multilayers remains the same on both ends of a chamber and only the relative position of the cross-plates glued between them is affected. Nevertheless the measurements show that Y differences are smaller than 20 μm on both Ref and NonRef side of the combs.

4 Machinery for Assembly and Gluing

To dispense the glue on the tubes we developed a gluing machine based on the concept described in [**?**]. The glue is always distributed on the tubes in the combs on the granite table. The distribution of glue is illustrated in Fig. 4, showing a cross section of a few tubes in a multi-layer.

For the central rope between neighbouring tubes held in the combs we use the thin glue Araldyte-DP2019 which nicely distributes itself around the 65 μm waist.

To glue these tubes to the previously layer on the spacer we use Araldyte-2011 which is more viscous and therefore the side ropes on the tubes retain their shape until the two layers are pressed together.

4.1 Sag Compensation

When suspended by the ears on the stacking towers the weight of the chamber causes the cross-plates to sag by up to 50 μm at the chamber ends and xx μm in the middle. The tube layer to

be glued is held flat in the combs and thus without sag compensation a change in relative layer distance along the cross-plates would be frozen in. The sags are removed by the sag compensation system acting on the longbeams wich are attached to the cross-plates at the Bessel points. This allows to reduce the sags by typically 90To be able to reach this value without the risk of lifting the spacer out of the sphere holders we added 10 kg weigths to the ears on the cross-plates.

The system consists of 4 pneumatic tower-pairs. Each pair carries a cross-bar that supports the two longbeams at a specific position. We use a pair near the outer cross-plates and a pair on each side of the middle cross plate. figure 4.1 shows two towers on the ref-side at the middle cross-plate, which form individually two pairs with their corresponding towers at the non-ref side of the chamber. The support of sag compension towers on the table allows them to move freely over several mm in the horizontal plane such that the spacer positionning is not constrained by the sag compensation.

5 Assembly Monitoring

5.1 RASAS system

The precise positioning at the level of 10 μm of the spacer (with tube-layers already on it) on the sphere holders is of crucial importance. Mis-positioning leads to layer-wise difference in the Y-pitch and Z-pitch.

To monitors the spacer position during the gluing procedure we developed the RASAS system. The RASAS towers are fixed to the granite table and accomodate a CCD en lense. Together with a mask embedded in the 'ears' on the spacer this forms a (standard) RASNIK system.

To translate the RASNIK coordinates into our Global Coordinate System we have to know the relative tranlation and rotation of the coordinate frames. The quantities directly measures by RASNIK are the position (X_R, Y_R, Z_R) and angle (A_R) of the mask with respect to the CCD-lens system.

The optical axis points roughly into the global X direction, RASNIK X and RASNIK Y point roughly in the global Z and Y direction respectively. The rotation around the optical axis of the mask, A_M, has to be known with an accuracy such that $\sigma_{angle} arm = \sigma_{position}$. When we aim for a calibration error of 5 μm , with the arm to be the largest step size of 26mm, we obtain $sigma_{angle} arm = 5\mu m/26mm = 200$ μrad . Other rotations of the mask can be ignored; these effect the results only at the second order level. The construction of the RASAS towers and ears, guarantee that these rotations are comfortably small (<25mrad). The precision on angle of the optical axis (CCD-lense) with respect to the global X axis in the global X-Y plane, A_{XY}, and X-Z plane, A_{XZ}, is set by possible movement in X of the spacer of about 10 mm. This leads to an accuracy of σ_{angle} = 5 μm /10mm=0.5mrad for A_{XY} and A_{XZ}.

The coordinate transformation can now be expressed in measurable quantities:

$$Z_G = X_R + Z_R A_{XY} + Y_R A_M - X_o f f set \quad (1)$$

$$Y_G = Y_R + Z_R A_{XZ} - X_R A_M - Y_o f f set \quad (2)$$

where the suffix R and G represent the coordinate systems RASNIK and Global respectively. Note that the CCD is treated as a point when the RASNIK coordinates are extracted. Therefore the CCD rotation ($A_{CCD} = A_R + A_M$) has not entered these equations.

5.1.1 Calibration Constants

Pre-calibration CCD rotation The rotation of the RASAS CCDs A_{CCD} with respect to the granite table are measured using a special precalibration tower equipped with a mask of known rotation. The RASAS- and precalibration towers are put on the granite table such that the mask image is properly projected on the CCD. The angle is measured by RASNIK to a high statistical accuracy. However, we observed that small movements of the towers lead to large fluctuations of the measured angle. These systematic effects are not completely understood and therefore we assign an uncertainty to the precalibration of 200 μrad corresponding to the size of these fluctuations.

The calibration of rotations The spacer is positioned in the central stacking position and the RASAS system is read out. It provides the RASNIK coordinates X_R, Y_R, Z_R and rotation of the mask A_R, relative to the CCD en lense system. Note that the rotation of the masks $A_M = A_{CCD} - A_R$ is already known to about 200 μrad , when we ignore the positioning error of the RASAS towers on the granite table.

The direction of the optical axis, represented by the angles A_{XY} and A_{XZ}, are determined by moving the spacer (and thus the masks) in the RASNIK Z (Global X) direction. The angles follow from the change in RASNIK readings as function of the movement in X using:

$$X_R = A_{XZ}X \tag{3}$$
$$Y_R = A_{XY}X \tag{4}$$

The uncertainty on A_{XY} and A_{XZ} is dominated by the uncertainty in the sphere tower orientation of about 0.5 mrad.

The calibration of off-sets There is no direct way to calibrate the absolute off-sets of the RASNIK system. For the assembly in general it is sufficient to check that all steps in Y and Z for the three stacking positions are reproduced within 5 μm . In this case the RASNIK readings in the central stacking position are used as off-set.

Consistency check We can position the spacer in all orientations, such that all four RASAS-masks are viewed once by the four RASAS towers. This provides information on the intercalibration of the mask angles. In addition, data obtained in all the stacking positions of the spacer contains information on the possible stacking block deviations and provides information on the absolute calibration of the mask angles. We attempt to extract this information in a fit procedure using the RASAS readings.

In the free parameters in the fit procedure are:

- the mask angles (4 param.),
- the Y deviations of the layer one and three stacking blocks (8 param.)
- the Z deviations of these blocks at the reference side (4 param.)

The residuals, see Table 5.1.1, amount only a few microns, consistent with the expected stacking reproduction errors.

The resulting mask angles are listed in Table 5.1.1. The mask angles, determined in the fitting procedure, are compared to the initial angles determined from the relative CCD-MASK angles provided by the RASAS systems and the precalibration of the CCD angles. We observe deviations, consistent with the systematic uncertainties of 200 μrad .

The block deviations are displayed in Table 5.1.1. These deviations are below 10 μm as expected from the CNC measurements desribed in Section ??.

5.2 RASNIK systems on the spacer

The In-Plane and Cross-Plate systems have all their components on the spacer, contrarily to the RASAS system which has its basis on the granite table.

The In-Plane system consists of four RASNIK systems and is described elsewhere [**?**]. This system will be used in the experiment to monitor the chamber deformation, but it constitutes a usefull monitoring system during the assembly of the chambers as well.

During chamber assembly the two outer cross-plates are equipped with a Cross-Plate system RASNIK system running parallel to the cross-plate. These systems monitor the reduction of the gravitational sag by the sag compensation system.

After the assembly of the bare spacer these systems are calibrated by taking the average of the readings in the 'up' and 'down' orientation in the central stacking position.

5.3 End-Plug Laser System

A commercial laser system is used to check the position of the endplugs held in the Frascati jigs before a layer of tubes is glued to the spacer. It consists of a laser sender producing a rectangular beam of 16x1 mm2 and a receiver which translates light input into voltage output.

The sender and receiver are mounted on base blocks of the sphere towers on either side of a Frascati jig, such that the rectangular laser beam is positionned above the precision rings of the plugs with the long side parallel to the Y axis. The height above the table is chosen such that 50endplug is placed in the wedge formed by two adjacent endplugs held in the Frascati jig. The relative size of the shadow determines the output voltage of the receiver. By scanning over all adjacent pairs of endplugs in the comb a misplacement is detected as a significant change in output voltage. Repeated positionning of the reference plug shows an intrinsic precision better than 4 μm . A more detailed description of the apparatus and the method can be found in ref.Guido.

The system has been calibrated by inserting steel foils of known thickness between the reference plug and the underlying tube plugs and comparing the change in height with the change in output voltage.

Both sides of the assembly table are equipped with such a system and the scanning is done simultaneously by moving a standard tube with reference plugs on both ends from wedge to wedge. The position of the reference along the comb is read out with a barcode reader scanning a ruler next to the comb, after which the voltages are read out. At the end of a scan the deviations from a straight line fit through the data are presented to the operator. The whole procedure takes about 15 minutes.

5.4 Automated assembly manager

To prevent mistakes and to automate the monitoring of the assembly procedure we use an 'assembly manager' embedded in a computer-programme.

The assembly manager presents the assembly step to be performed by the crew in text and pictures. Before each step it checks whether it is allowed to perform the step based on

- temperature measurement of the environment, table and spacer,
- vacuum of the tube-suckers,
- pressure readings from the sagcompensation system.

After each check it checks te result of the relevant system, such as:

- RASAS, In-Plane and Cross-Plate RASNIK readings,
- Guido-Laser system

During glue-curing it monitores the environment continuoully and generated warnings (emails) in case of attention is needed.

It also generates output for to evaluate the quality of chamber under construction.

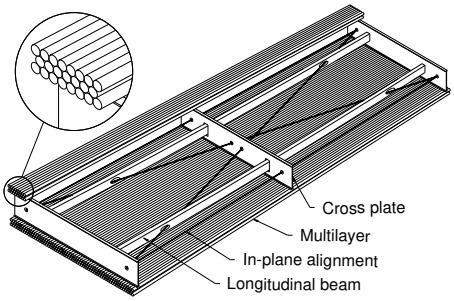

Figure 1: *Schematic view of a muon chamber.*

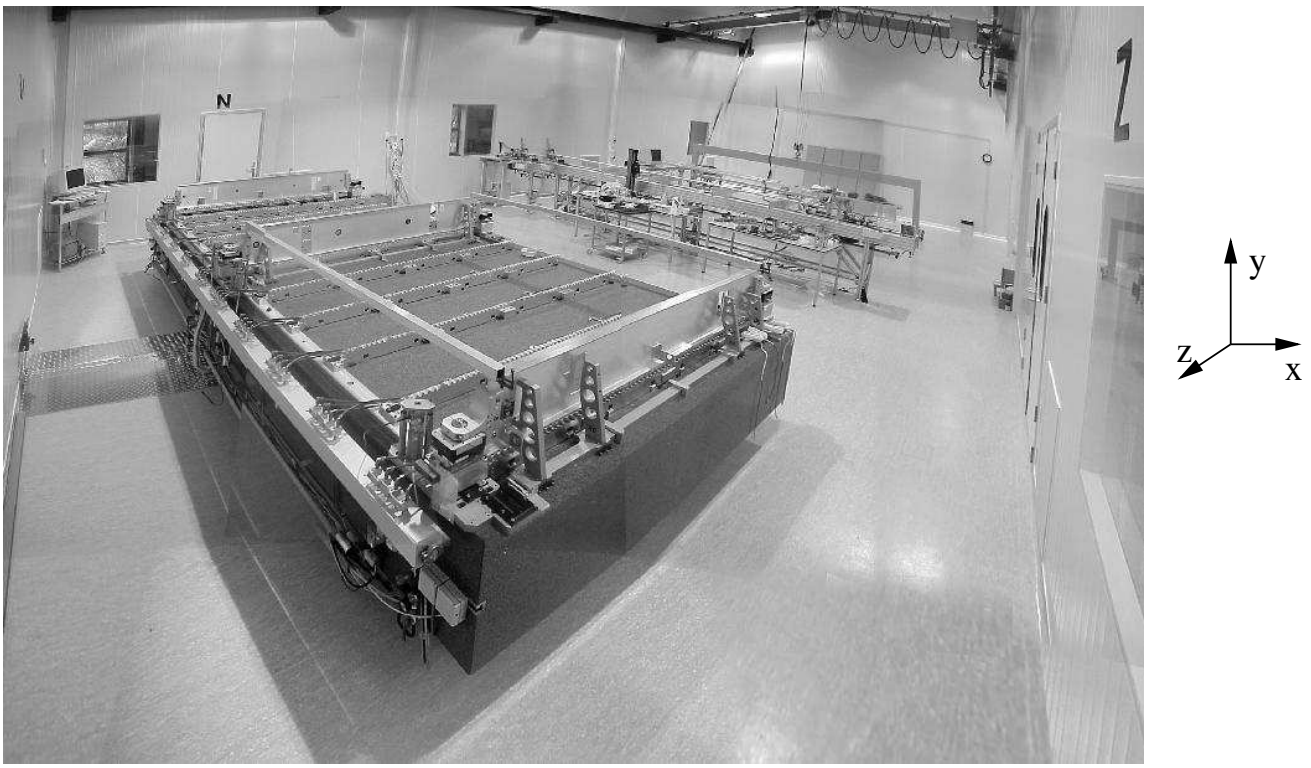

Figure 2: *View of the assembly station. The bare spacer is carried by the six sphere towers. The combs, which will support the tubes are also visible. In the background, the tube production can be seen. The coordinate frame is also displayed in this figure; on the wall the character 'N' defines the 'North' direction, which coincides with the X direction.*

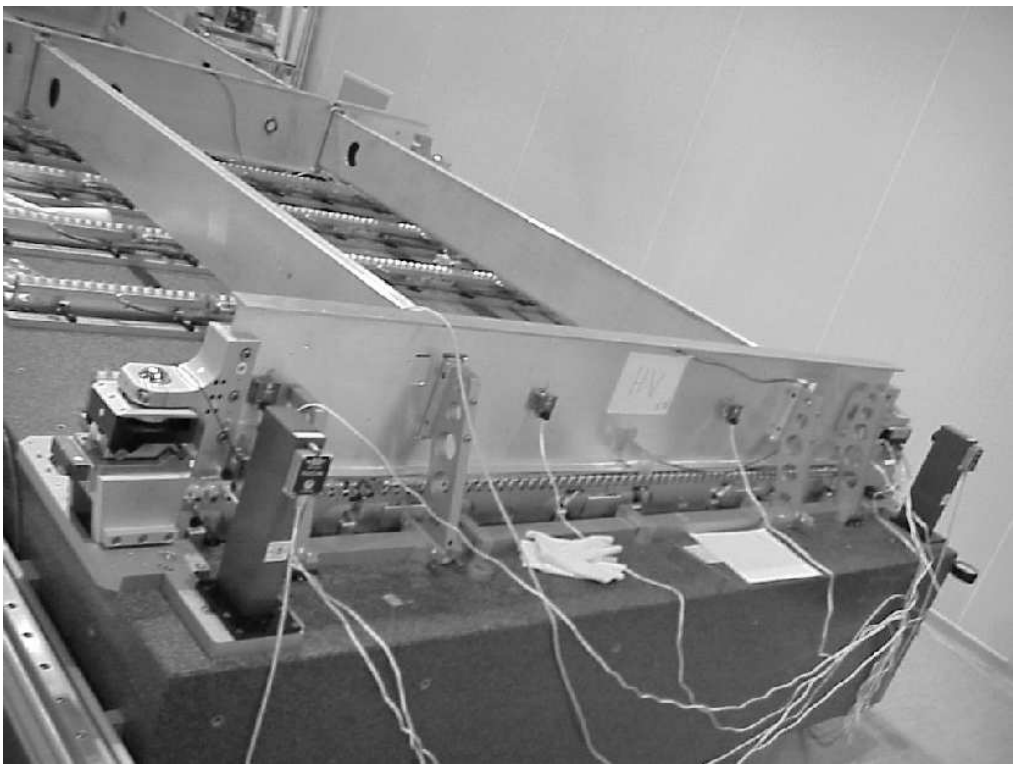

Figure 3: *The picture shows one sphere tower that carries the spacer. The 'removable' ear on the spacer is monitored by the aligment system.*

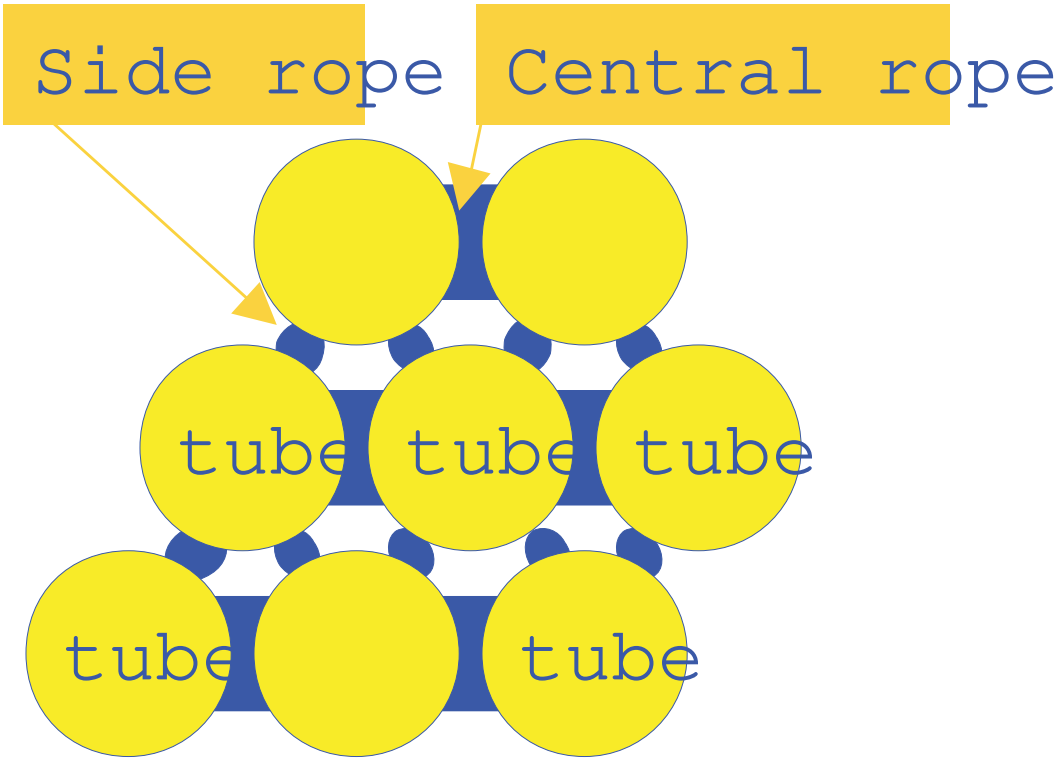

Figure 4: *Glue distribution between tubes in a multilayer.*

Figure 5: *Two sagcompensation towers at the middle cross-plate.*

		dY				dZ		
Position	**RASAS**	**layer 1**	**layer 2**	**layer 3**		**layer 1**	**layer 2**	**layer 3**
A+	NW	**0**	***0***	**0**		**0**	***0***	**-1**
A+	NE	**1**	***0***	**1**		**-3**	***0***	**1**
A+	SE	**0**	***0***	**0**		**-1**	***0***	**3**
A+	SW	**1**	***0***	**0**		**1**	***0***	**1**
C+	NW	**1**	***0***	**2**		**2**	***0***	**0**
C+	NE	**0**	***0***	**0**		**3**	***0***	**5**
C+	SE	**0**	***0***	**1**		**-2**	***0***	**-1**
C+	SW	**0**	***0***	**-1**		**0**	***0***	**-2**
A-	NW	**-2**	***0***	**-1**		**0**	***0***	**-3**
A-	NE	**-2**	***0***	**-1**		**-1**	***0***	**2**
A-	SE	**-1**	***0***	**-1**		**1**	***0***	**1**
A-	SW	**-1**	***0***	**-1**		**1**	***0***	**-1**
C-	NW	**1**	***0***	**0**		**0**	***0***	**-3**
C-	NE	**0**	***0***	**-1**		**0**	***0***	**0**
C-	SE	**0**	***0***	**0**		**-1**	***0***	**0**
C-	SW	**1**	***0***	**1**		**1**	***0***	**-2**

Figure 6: *Results of the Grand Fit*

fitted angles			**Deviations**		
			A+	**C+**	**A-**
Mask 1	**-4.04**	**NW**	**0.21**	**0.09**	**0.07**
Mask 2	**-3.67**	**NE**	**-0.03**	**-0.18**	**-0.11**
Mask 3	**-1.54**	**SE**	**-0.04**	**-0.31**	**0.03**
Mask 4	**-0.63**	**SW**	**-0.02**	**0.13**	**-0.21**

Figure 7: *Results of the Grand Fit*

Blocks	dY				dZ	
	layer 1	layer 2	layer 3		layer 1	layer 2
NW	-4	0	5		1	0
NE	-9	0	-1		1	0
SE	-6	0	0		-4	0
SW	0	0	3		-4	0

Figure 8: *Results of the Grand Fit*

6 Assembly Procedure

The assembly station allows in principle to produce chamber with a precision below 20 μm (of the wire positions). To build about 100 (similar) chambers in a few years with a few persons, a fast production procedure with quality monitoring during the essential steps is necessary.

The speed of the production is limited by the glue curing of the spacer, which takes a nigth, followed by the gluing of the tube-layers in six subsequent days. The monitoring of the spacer position and that of the end-plugs are of the highest importance. Additionaly, the gravitational deformation of the spacer (with tuber-layers on it) has to be compensated and monitored.

6.1 Assembly of the bare spacer

The spacer parts, the two longbeams en the three crossplates, are put together on the granite table. The precision of the bare spacer can be as low as 500 μm , far below than the precision of the granite table. However, the sag-compensation, RASNIK and other facilities available at the granite table are used during the spacer assembly.

During the first day the RASNIK components (see Fig. 6.1), temperature sensors and cable guides are mounted and fixed. The longbeams are positioned at by temporary mechanics and supported by the sagcompensation system to remove the gravitational sag. We use a pressure corresponding to 50% for the centre and 25% for the outer compensation towers of the weight of the longbeams.

After the overnight glue curing the RASNIK systems (in-plane, cross-plate and also RASAS) on the spacer are calibrated. For the in-plane alignment system we use the central stacking position and take the average of the up and down orientation. For the RASAS system we take reading in all stacking positions and up/down orientation and set all offsets individually to zero. Dedicated calibration software checks the internal consistency of all the readings. Additionally a comparison is made with the calibration values of previously build chambers. The rotations, Y values and the ref-side Z values give strong indications when something is wrong. The RASNIK reading (which were set to zero to faciliatate their interpretation by the assembly crew members) should now be reproduced within 10 μm during the assembly.

After the spacer has been assembled the In-Plane calibration tower (see A) is placed in front of the four in-plane masks. From these readings we obtain the absolute orientation of the in-plane masks. At the end of the chamber assembly, final measurements with the 'airborne' spacer in 'up' and 'down' position provide a consistency check as described below.

6.2 The gluing of tube layers

The wire tension of the tubes are checked just before the tubes are used for a new tube-layer. Then the tubes have to be properly positioned in the jigs. Although this appears straitghforward, only experienced crew members have developped enough feeling to perform this task flawless.

In the longitudinal direction the gas-jumpers are temporarily mounted to aling the tubes such that length differences (which amount 200 μm on average) are absorbed. The orentation of the tubes is controlled by a smal orientation pin, contrained by the North-side tube-comb. Finally, the tubes are sucked to the combs by small vacuum suckers. the procedure is checked by the Guido-laser system, discussed below.

Glue is dispensed (see 6.2) between and on the raakvlakken of the tubes for the first two (and

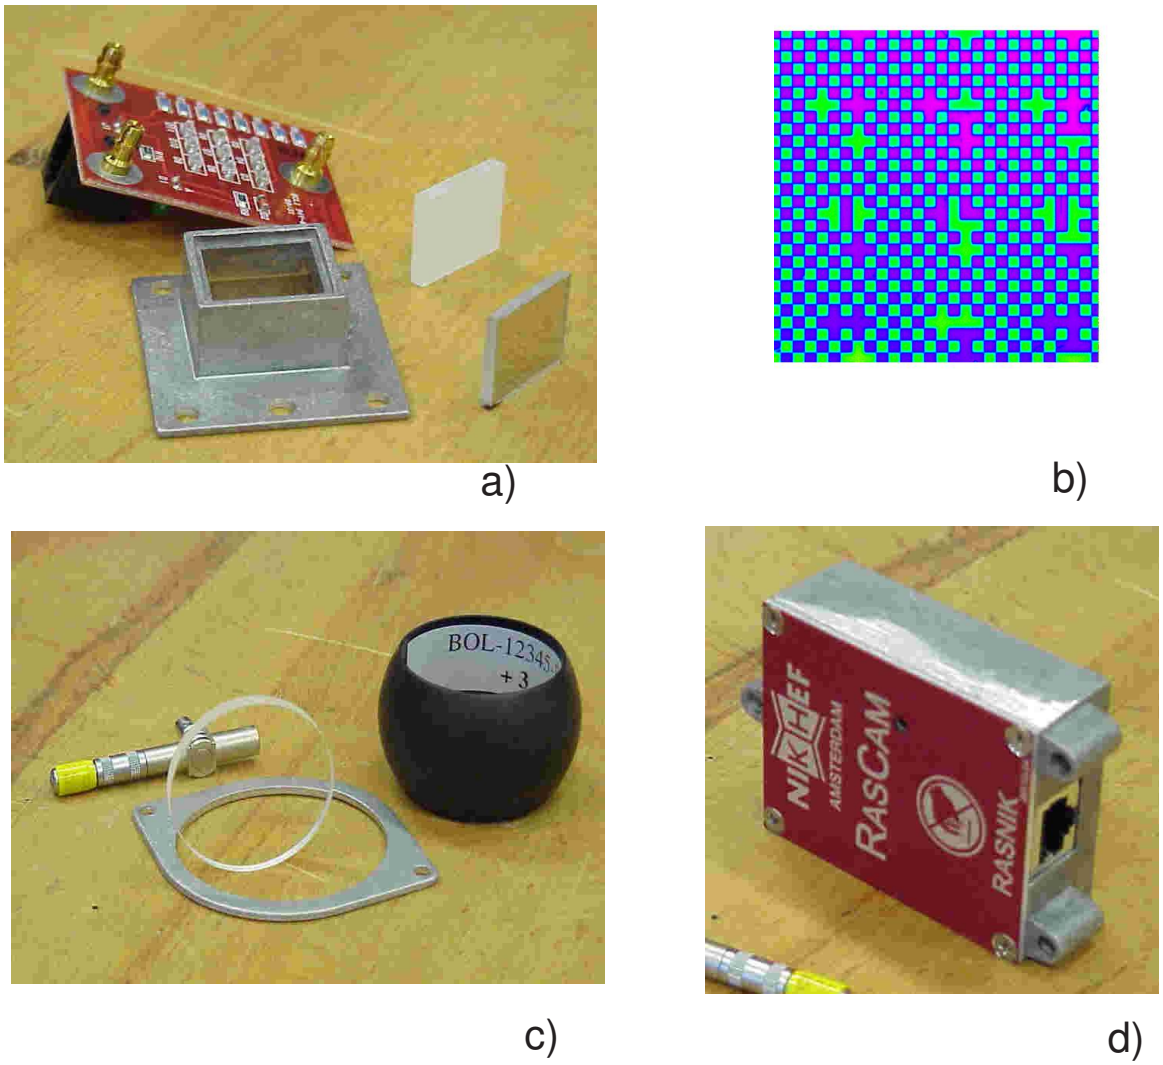

Figure 9: *a) Picture of the RASNIK-Mask components. b) The mask-image as seen by the image sensor (CCD). c) Pictire of the lense and its holder. d) Pictucer of the housing of the CCD*

following) tube layers. The spacer is lowered to the tubes (see Fig. 6.2) and the sagcompensation system is turned on. We use pressures that corresponding to about 90% of the weigth of the spacer (and the layers glued on it). To avoid an assymtric (tube-layer) weigth distribution, we flip the spacer between the glueing of tube layer 1-2, 3-4 and 5-6 by rotating over its Z axis (its 'short' symmetry axis in the horizontal plane).

Figure 10: *Glue is dispensed on a tube layer by the gluing machine.*

7 Control of chamber assembly

The strict quality control is essential to keep the precision and quality of the chambers at a constant and high level. Various checks are performed by the assembly crew. The vital checks use automated montoring systems which were introduced in Section 5. Our experiences with these systems will be presented in this section.

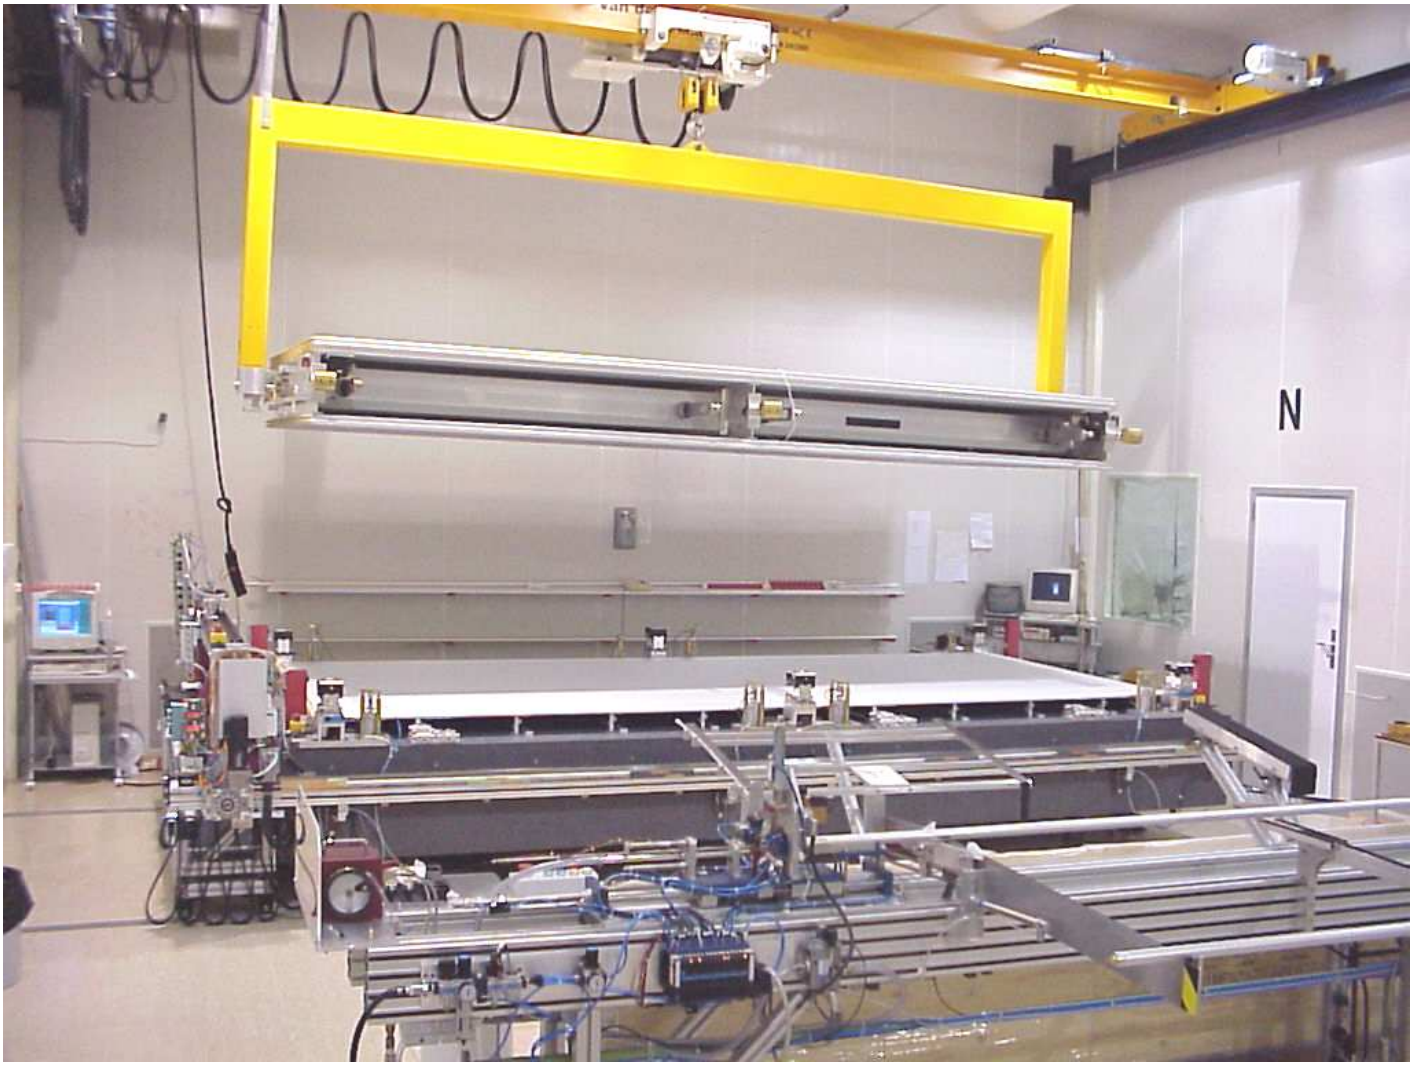

Figure 11: *Lowering of the spacer with some tube layers already on it, on a tube layer on the granite table.*

Figure 12: *Picture of the finished BOL0 chamber.*

7.1 Control of the tube position

The position of the tubes placed in the jigs is checked prior to glueing by the readings of the End-Plug Laser systems at HV and RO ends (see 5.3). A typical example of the residuals from a straight line fit throught the data is shown in fig [gltyp.ps]. Deviations of more than 20 μm require an inspection of the associated tube(s). Repositionning of the tube usually solves the problem. Only in a few cases tubes had to be replaced because the plug was inproperly crimped into the tube. So far no significant deviations caused by plug diameter variations were found.

In Fig **??**a and b we plot the average of the residuals from the straight line fits for all 6 layers of the first 4 chambers as a function of the position in the comb at each side of the assembly table.

The error bars represent the rms of the 24 deviations found at that position, typically 5 μm . Systematic deviations of order +-8 μm can also be recognised. These are attributed to the fact that the jigs are assembled out of 4 solid pieces which were precisely machined and then glued together. The fixation of the jigs to the granite table and to the assembly stacking towers on the reference side (position zero in the plots) also leads to small distortions. However these systematic deviations are well within the required precision.

7.2 Layer-pitch control

The relative position of tubelayers is determined by the precise geometry of stacking blocks in the assembly jig and the positioning of the spacer on these blocks during glueing. This position is monitored by the RasAss towers at each corner of the chamber. In addition the sag of the HV and RO cross-plates affects the layer distance inbetween the stacking towers. This sag is controlled by the sag compensation system of the assembly jig [see Assembly.SagComp] and monitored by the XP-Rasniks. We tested the machinery for BOL0 by measuring the sag of the (non) compensated cross-plate with the Heigt-Meter and compared the results with the RASNIK measurements. The results are shown in Fig. 7.2, together with the predicted sag based on a FEA. From these results we conclude that we control the cross-plate sag below the level of 20 μm .

The position and sag of the middle cross-plate is inferred from monitor data of the Inplane Rasnik system mounted on the spacer, but this only concerns the relative position of the tubes, not the wires.

7.2.1 Layer Z-pitch

In fig[zshav] we plot for chambers BOL0 to BOL8 the RasAss deviations from the zero z-position at the end of a glue curing period of typically 16 hours.

The points shown are the deviations seen by the reference-side RasAss-towers at the HV- and RO-ends respectively. Temperature effects can be neglected on the reference-side since the distance from the stacking block fixing the z-position to the mask of the rasnik system on the cross-plate is only 14cm. During curing the corresponding Rasnik values are found to be stable within +- 2 μm (see also Fig. 7.3). In contrast the z-values at the non-reference side fluctuate by typically +-5? μm as a consequence of small temperature (+-0.1? deg) variations and the 2m length of the cross-plate. When corrected for, by using the temperature sensors mounted on the cross-plates, the z-positions at the two sides are found to be consistent within ?? μm .

The data are plotted separately for each layer within a multilayer at the HV- and RO- ends. In addition a histogram of all deviations is shown. As can be seen, all positions are well with the

desired range, except for the first two chambers. For these chambers the 'spacer landing-gear' of the assembly jig (see [Assembly.LandingGear]) was not yet installed, and consequently spacer-positioning was not as precise due to resistance of the glue in between the tubes.

7.2.2 Layer Y-pitch

In fig[yshav.ps] we plot for chambers BOL0 to BOL8 the deviations from the nominal y-pitch (26.011mm) as expected from the Rasnik monitor data and the CNC measurements of the layer-stacking blocks (deviations +4 μm). The Rasnik deviations are calculated by taking the average deviation from the calibration values of the East- and West-side RasAss-towers at the HV- and RO-ends respectively and adding 2/3 of the cross-plate sag as observed by the XP-Rasniks (assuming a parabolic sag of the cross-plate).

The data are plotted separately for the inner(layer12) and outer(layer23) layers within each multilayer. Furthermore the data is shown at the start of the layer-glueing(Wet) and after the glue has cured (Dry).

As can be seen the layer pitch of the inner layers is of the order of 20 μm larger than nominal after the glue has cured, while it is much closer to nominal at the start of glueing. We attribute this to the shrinkage of the particular glue [XXX] that is used to glue the innermost layers to the spacer. For this glue we observed in a simple test a shrinkage of the order of a few permille??. This can explain the observed change in layer distance over time, considering that the distance between the cross-plates and the tube-layer.

A typical example of RasAss and XPAss Y-values versus time are shown in Fig. 7.3 for the glueing of the first 4 layers of the BOL8 chamber.

In contrast the layer pitch of the outer layers does not change during curing of the [YYY] glue used for these layers. In this case the distance between the tubes in the two layers is of the order of 70 μm and no obervable shrinkage effect is expected. For the outermost layers the average pitch deviation is +5 μm with an rms of 5 μm .

7.3 Relative positioning at the middle cross-plate

In fig[hismid.ps] we plot the deviations from the nominal layer pitch in z and y, for all the Inplane Rasnik readings (4 per chamber and layer). The results show that the relative position of the tubelayers in the middle of the chambers is centered at the nominal value with an rms of less than 10 μm in both directions. This is well within the required precision in order to satisfy the criterium that the wires must be whithin 100 μm rms at the centre of the tubes, as the mechanical precision of the middle stacking blocks is also of order 10 μm (see [AssJig.par]).

We conclude that the layer glueing is controled within +-5 μm in z and y and that fixed geometry parameters for the BOL chambers as presented in table [Tomo.sitep] can be assumed with a negligible effect on the muon momentum resolution. Wat doen we hiermee?

7.4 Final measurements

For each chamber we perfrom a final measurement 'in the air'. We take measurements in the 'up' and 'down' orientations of the airborne spacer.

The gravitational sag of the chamber amounts about ∓ 1.8 mm in the 'up' and 'down' position respectively. An assymmetry in the 'up'/'down' sag points to a problem in the sagcompensation procedure. Sofar we found no deviations beyond the level of 10%, which is the accuracy of sagcompoensation system.

From the change of the in-plane readings and the reasonable assumption that we introduce a pure sag in the Y direction, the mask angles can be simply obtained from dX/dY. This provides a check on the calibration of the in-plane mask angle with the calibration tower described above.

8 Results of X-ray scans

The mechanical accuracy muon chambers is checked in the X-ray tomograph at CERN. All types, but about 10% of all chambers, are certified by this device.

Here we discribe the tomograph briefly, a detailed description can be found elsewhere [**?**]. The tomograph consists of a unit with two X-ray beams that runs over the chamber in the Z direction. The shadows of the beams is measured with scintillator counters. From the pattern of these shadows, the wire positions can be extracted with an accuracy better than 10 μm .

Figure 8 presents a 'wire-map' of the chamber near one of the outer cross-plates.

In Fig. 7.1c and d we plot the residuals from straight line fits throught the data of the X-ray tomograph scans for BOL0. In this case the data from individual layers in each multilayer at the HV and RO side are combined such that they correspond to the same side of the assembly table at which they were glued. In this case the error bars represent the rms of the tomagraph data at each tube position. The systematic deviations in the X-ray data are clearly correlated with and of the same size as the planarity laser data. This shows that tube positionning and its QA are well under control.

In Fig. 7.3 we compare the z deviations described above with those obtained from the analysis of the X-ray tomograph data for chambers BOL0,BOL2 and BOL3. In order to compare different multilayers, the Rasnik deviations are shifted such that the average deviation is zero for the HV- and RO-side respectively. This corresponds to the combined fit applied to the tomograph data for a scan through each end of the chamber with the zero position taken at the middle between the two multilayers. The two sets of data ar nicely correlated with an rms of the difference of 6 μm .

In Fig. 7.3 we compare the Y-pitch deviations described above with those obtained from the analysis of the X-ray tomograph data for chambers BOL0,BOL2 and BOL3. The two sets of data ar nicely correlated with an rms of the difference of 7 μm .

Table 1 gives the RMS for....

	BOL0	BOL2	BOL3
Rms Z (μm)	15	12	13
Rms Y (μm)	13	17	14

Table 1: *The RMS results.*

The site parameters are listed in Table 2.

	Nominal	NIKHEF
Z-pitch	30.035	30.0353
Y-pitch	26.011	26.027
dY-Multilayer	399.032	398.984

Table 2: *The side parameters extracted from a the tomograph scans of BOL0.*

9 Further investigation and Additional Checks

To evaluate the quality of the produced chambers several studies were performed. All checks indicate that the chambers are produced according to their specifications. some of the checks are discussed below.

9.1 Tube layer pitch

Tube layers already glued to the spacer are only held at the ends and in the middle and thus will sag in between, touching the tubes of the next layer to be glued which are held in a plane by the 11 combs. As the outer tube diameter is 65 μm smaller than the wire pitch the layer distance between touching tubes will not be the same as the layer distance between wires and moreover the effect is cummulative when the third layer is added..

To reduce this effect strips of 50 μm thick scotch tape are put on the (next) layer of tubes lying in the combs . Since this requires non-trivial adjustments to the automatic glueing machine to avoid interference of glue ropes and strips and additonal labour for each glueing step, we tried to minimize the extra work.

In fig [multidik.ps] we show the results of measurements of the total thickness of the multilayers measured at several positions between the crossplates. For this we used a schuifmaat and only the sides of the two multilayers can be measured. The data are plotted as average deviations from the nominal value (61.922 mm) at approximately 25cm intervals along the length of chamber starting from the RO side.

The first trial was on the BOL0 prototype with 2 strips applied over the full width of the chamber between the Middle and HV cross plates and no strips between Middle and RO. As can be seen in the plot (black line) , the strip side deviates by 50 μm and the no strip side by 120 μm , Although the strips clearly help in reducing the effect, applying strips over the full width of the chamber cannot be done on the assembly table. The spacer has to be lifted in a vertical position next to the table to put the tape on the layers already glued to it. This is potentially hazardous and time consuming. Consequently the choice was made to put strips in regions spanning 10 tubes near the sides and near the long beams at 1/3 and 2/3 of the distance between middle and outer cross plates. This can be done quickly on the table after the glue ropes are laid. The corresponding measured average deviation is about 80 μm (green line in fig).

9.2 Temperature Gradients

The chambers are constructed from aluminium that expands typically 24 μm /m/K. Ovrall temperature changes are not seen by the RASNIK systems, but are monitored by the temperature sensors and can relatively easy be corrected for. In contrast, temperature gradients are more diffi-

cult to monitor and to correct for. In addition, the expected temperature gradients in ATLAS are not well predicted. Estimations vary, but over a chamber, between two multilayers, we should be prepared for gradients of 1 K. This implies that the chamber should not sag more that 100 μm /K to keep the wire sufficiently centrered and the cross-plate should not sag more than 20 μm /K. Of course, the gradient over the cross plate is monitored by the temperature sensorers and the effect is also seen to some level by the in-plane alignment, but we wish to avoid large corrections.

We conducted an small experiment by covering the BOL0 chamber (in its horizontal position) by electrical heat blankets. These blankets produce 50W/m^2, leading to gradients of several degrees. Figure 9.2 shows a side view of the chamber and the location of the temperature sensors. Figure 9.2a and b show the Y readings of the in-plane and cross-plate RASNIK system respectively during heating.

From the measurements we extract the values listed in table 3. for the chamber and cross-plate sag we obtain 50 μm /K and 6 μm /K which is well below our requirements.

Quantity	Effect	Effect Normalised to 1K over ML
T gradient over multilayers	4K	1K
T gradient over cross-plate	$\approx$0.3K	0.1K
T gradient over tube-layers in ML	$\approx$0K	0K
Chamber Sag	200 μm	50 μm
Cross-Plate Sag	25 μm	6 μm

Table 3: *The effects of heating the BOL0 chamber using electrical bleankets.*

10 Conclusions

chambers are within specs.

A Measurement tools

In this section we describe the home-made and other not so common tools to measre the mechanics and to align the assembly station.

A.1 The Heigth-meter

The heigth-meter is a commercial instrument to measure relative heights. It has an intrisic accuracy of 1 μm .

A.2 The malmonitor

The malmonitor is a homemade instrument to monitor the distance between NIKHEF sub- combs before and during gluing. A NIKHEF comb consists of four sub-combs.

The malmonitor consists of two parts which are placed on the two adjacent sub-combs. Two RASNIK systems are used to measure the possible shifts and also rotation between these parts with an accuracy of about 5 μm .

A.3 Laser optics

We use a Hewlett Packard laser with small (hardly visible) divergence over the relevant distance up to 6 m. Several optical instruments are used to measure angles, distance and straigthness to high accuracy. Instincically, the distance and straigthness measurement is accurate to a few micron; the angular measurement is accurate to 10 urad.

However, The obtained accuracy of the measurements is limited by the flatness of the contact surface of the mechanics and instruments and other reproduction errors.

A.4 Silicon Sensor

To measure the straightness we use a silicon sensor with strips in both tranverse directions with a pitch of 400 μm with respect to a laser beam. The sensor is mounted on a brass support with steel inserts which are positionned on small steel rods lying in the wedges of the combs. The laser beam position is obtained from the centre of gravity average of the strips with an accuracy of about 20 μm .

A.5 Bol-monitor

The 'Bol-monitor' consists of a cross-plate with two small lenses attached to one of the flanges approximately 1.8m away from each other. at positions corresponding to two precision wedges in the combs. This cross-plate is positionned on the stacking towers in the same way it is done for glueing tube layers. The relative position of each of the lenses is measured with an Mask/CCD-camera combination mounted on a brass fork with steel positionning inserts. This fork is placed on two precise steel rods lying in the jig wedges such that the cross plate lens is hanging aproximately in the middle between the Mask and the CCD. With the thus created RASNIK system the the lens position in Z and Y is read out , while varying the fork position by +-2mm in the optical axis direction (X) along the supporting rods. These measurements are done at both precision combs, using the same fork/rods combination. Comparison of the measurements yields the difference in Z and Y of the jig and reference assembly tower combinations. The use of two lenses on the cross-plate provides two independent measurements. In addition the whole procedure is repeated with the cross-plate rotated 180 degrees around the vertical axis, thereby interchanging the lens/fork combinations and yielding additional redundancy. The BOL-monitor was used to fix the initial position of the towers and the measurements will be repeated regularly as part of the QA/QC procedures.

A.6 Calibration tower for RASAS system

To calibrate the CCD rotation RASAS system we constructed a calibration tower with similar dimensions as the RASAS towers, but equipped with a mask. The idea is to fix and/or determine the rotation of this mask once, after which the tower can be used to calibrate the towers of the RASAS system. To determine the rotation of the mask in the calibration tower we use a 3D

measuring device with additional RASNIK tooling. This setup also allows to compare RASNIK and the 3D measurement device over a large range to the micron level.

The 3D measuring device is equipped with a platform holding a CCD en lense, which together with the mask in the calibration tower form a complete RASNIK system. The calibration tower is positioned on a granite table. The RASNIK response corresponding with a well controlled and known movement in Y of the 3D device allow to extract the mask rotation. In fact, the (small) rotation follows directly from the ratio of horizontal and vertical changes of the RASNIK readings, dX/dY. Both the 3D measuring device and RASNIK have measuring errors less than a micron. Thus, a measurement of the mask rotation is intrinsically accurate to about 1 μm /52mm=20 μrad .

The 3D device is moved vertical (Y) over a distance of almost 60mm. We observe that the change in the Z-reading of RASNIK, which represents the distance between MASK and CCD is constant within 10 μm , which implies that the angle between mask and an imaginary optical axis can be ignored. The first measurements are used to reposition the mask in the calibration tower, attempting to eliminate as good as possible all rotations of the mask. The mask is then fixed, actually glued, in the calibration tower. The Y readings of the 3D device and RASNIK are consistent over the full range as shown in Fig. refrasnik3d.

Now, we can study the residual variation of the X reading of RASNIK, which are related to the (small) rotation of the mask over the optical axis. The variation of X amounts only a few micron over the full range of Y as shown in Fig A.6. Finally, from a line-fit we obtain a rotation of 45 μrad +- 8 μrad . The measurement was repeated at several X positions, leading to consistent results. The flatness of the granite table is expected to be the dominant error contribution. To study we repeat the measurements for different positions of the calibration tower on the table and find an error contribution of 20 μrad . Additionally, when the calibration tower is used in situ, the flatness of the corresponding granite table adds to the uncertainties.

A.7 Calibration tower for In-Plane masks

To calibrate the orientation of the in-plane masks we equipped a tower of the appropriate heigth with a RASNIK lense and CCD. The intrinsic orientation of the CCD was calibrated using the RASAS calibration tower and found to amount 11.7 $\pm$0.11 mrad.

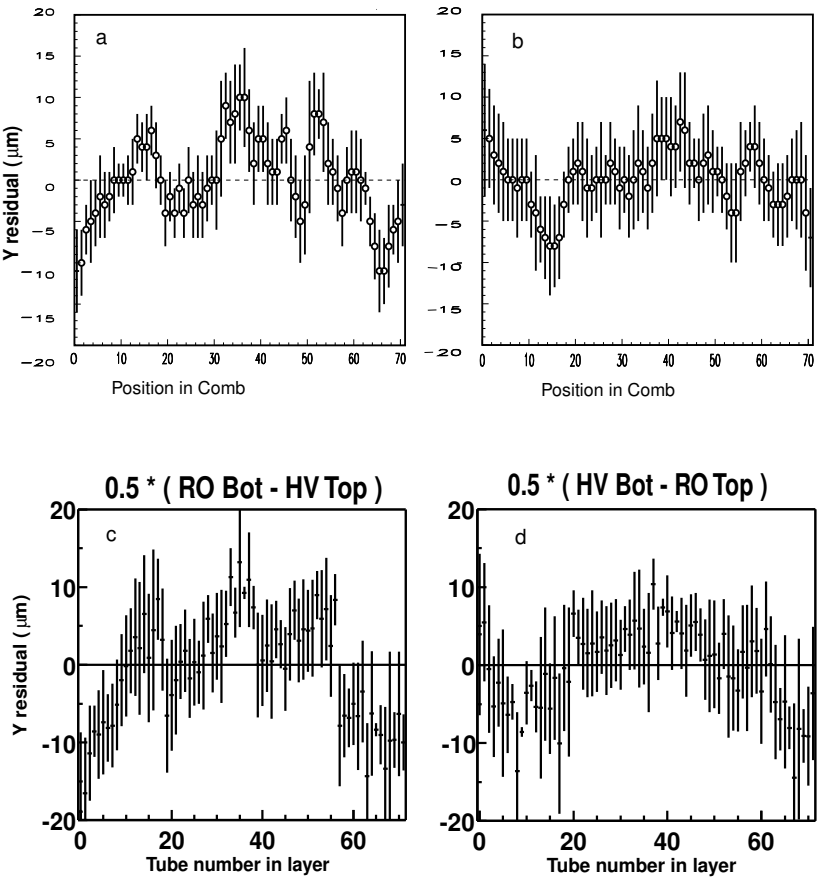

Figure 13: *a) b) Guido. c) d) tomo*

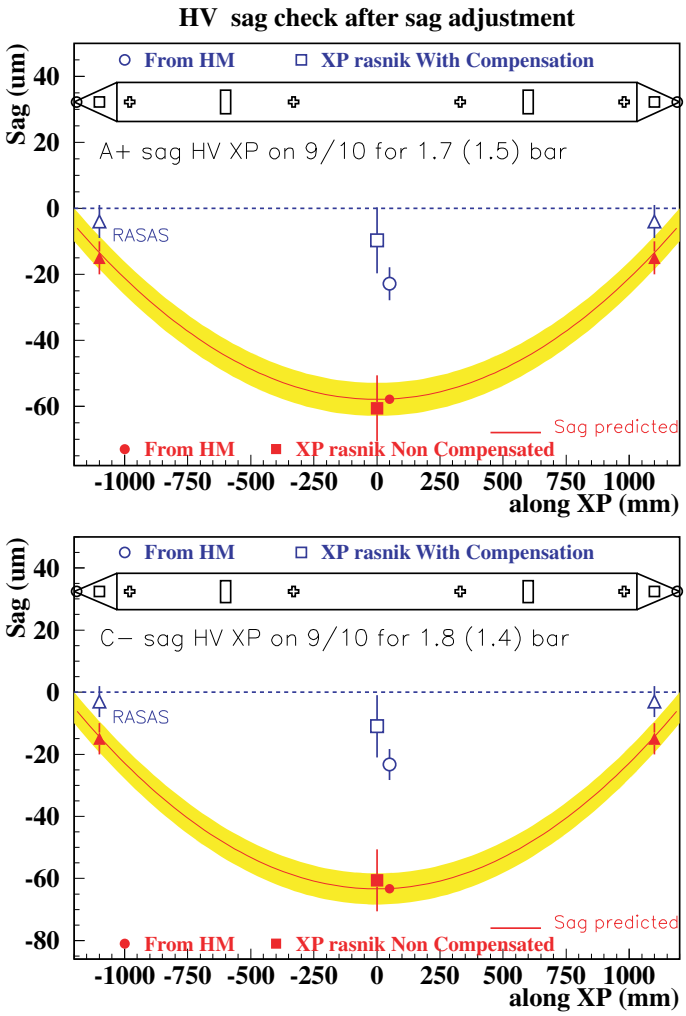

Figure 14: *The cross-plate sag as function Z. The band represents the predicted sag based on a FEA. The measurment from the Heigth-Meter (HM) and those of several RASNIK systems are also shown. The upper (lower) plot presnt the results for the 'up' ('down') orientation.*

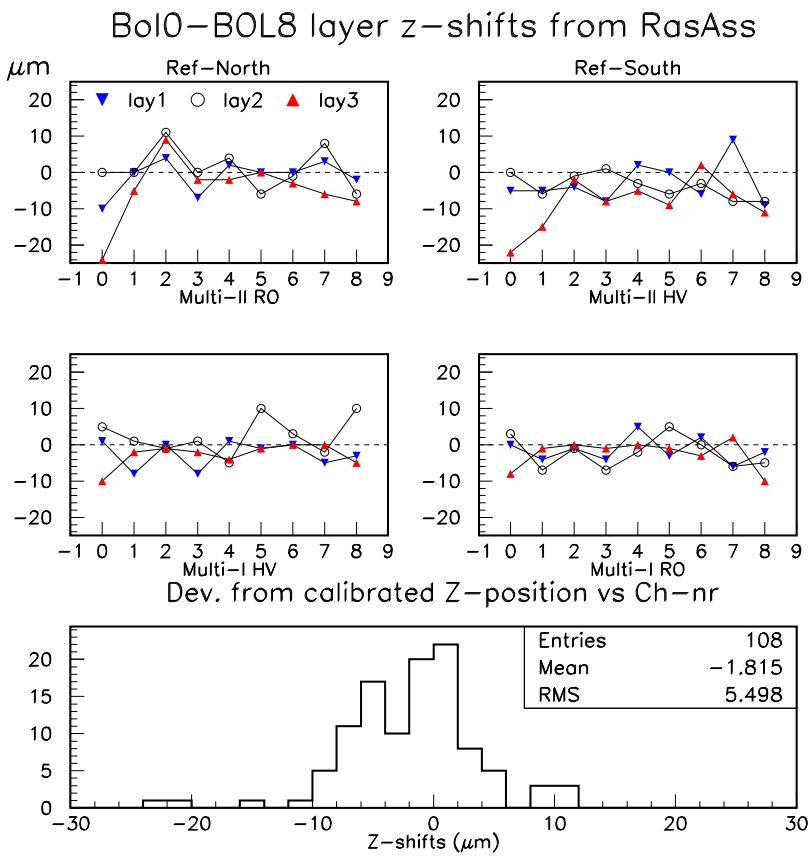

Figure 15: *Z shift av*

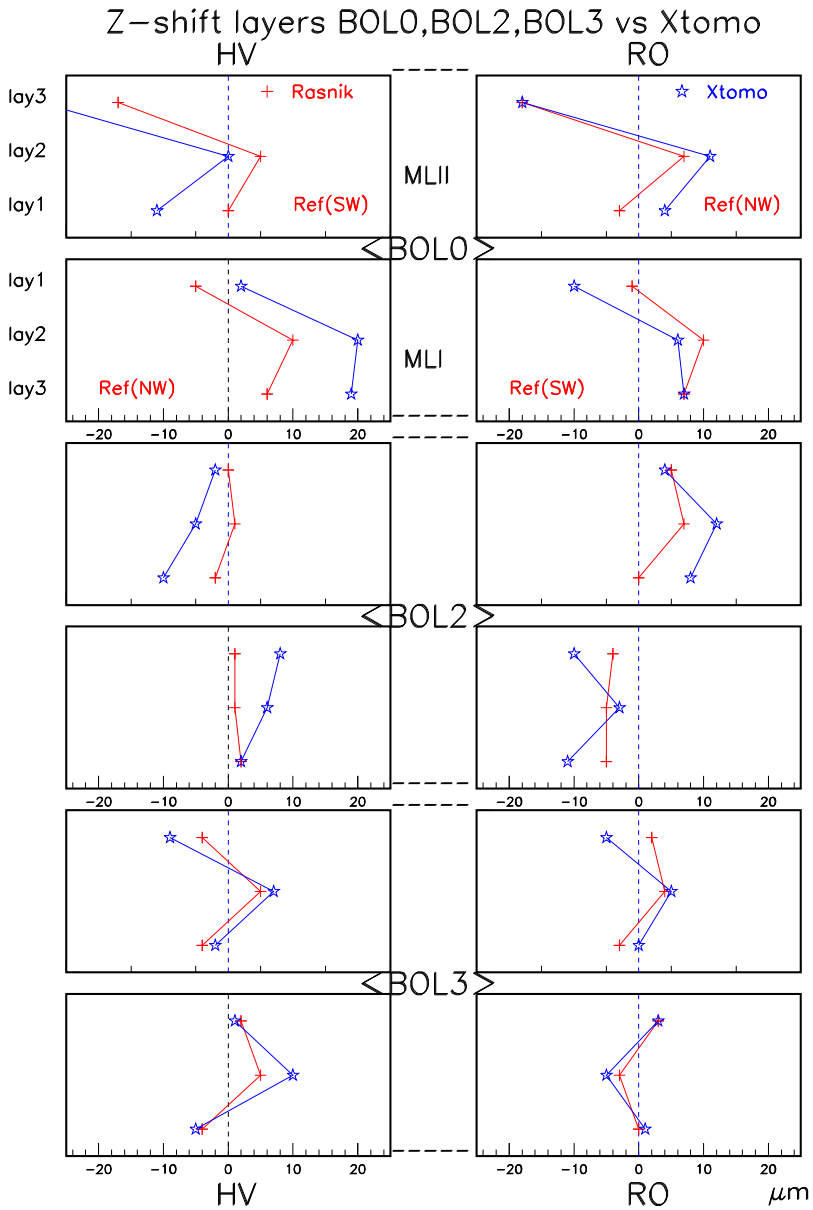

Figure 16: *z tomo and ras*

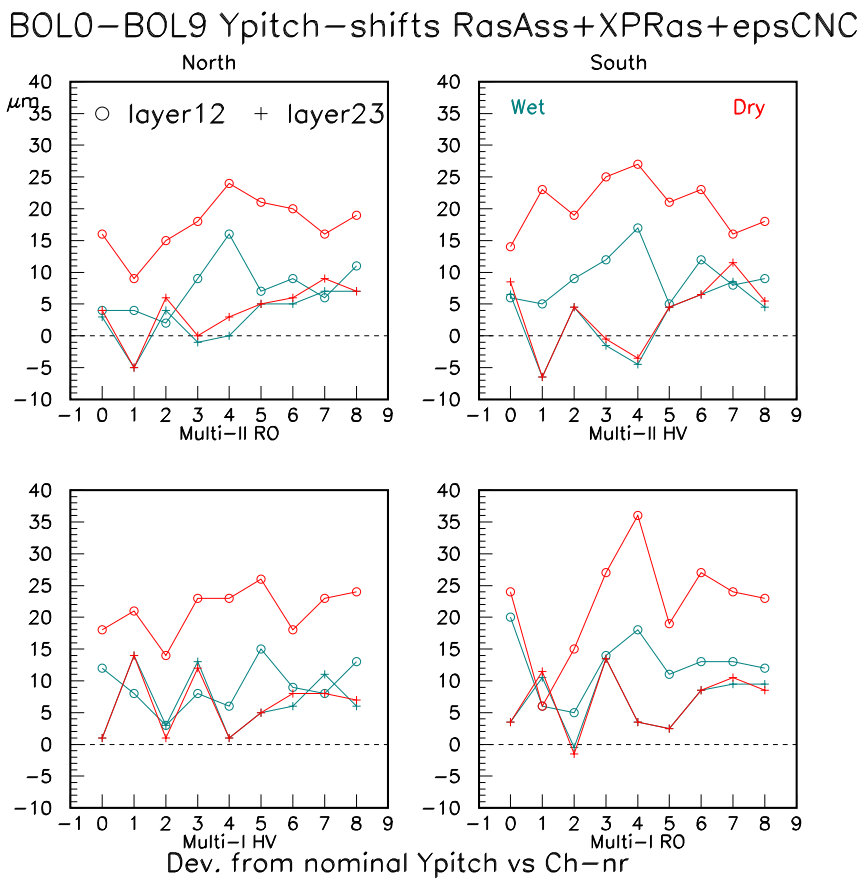

Figure 17: *y shift av*

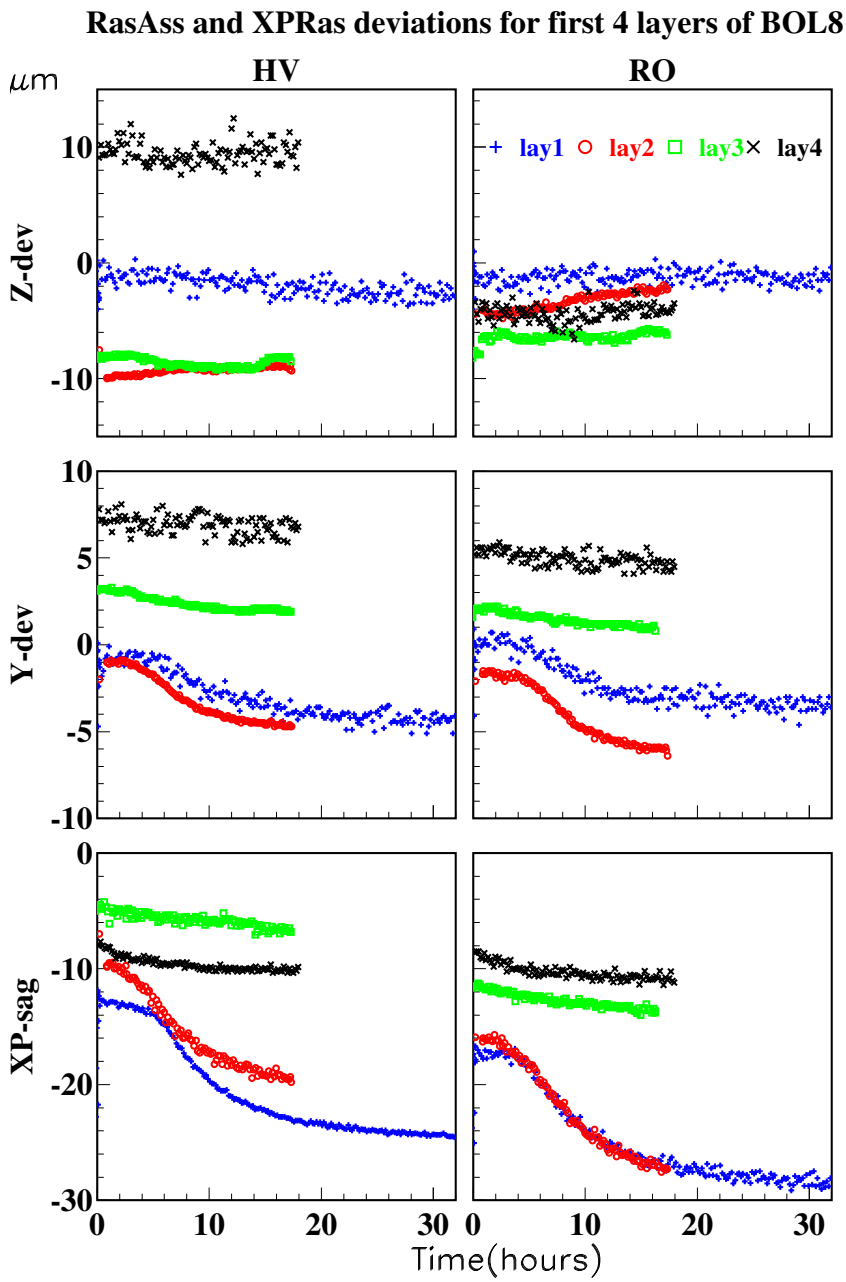

Figure 18: *mooi toch*

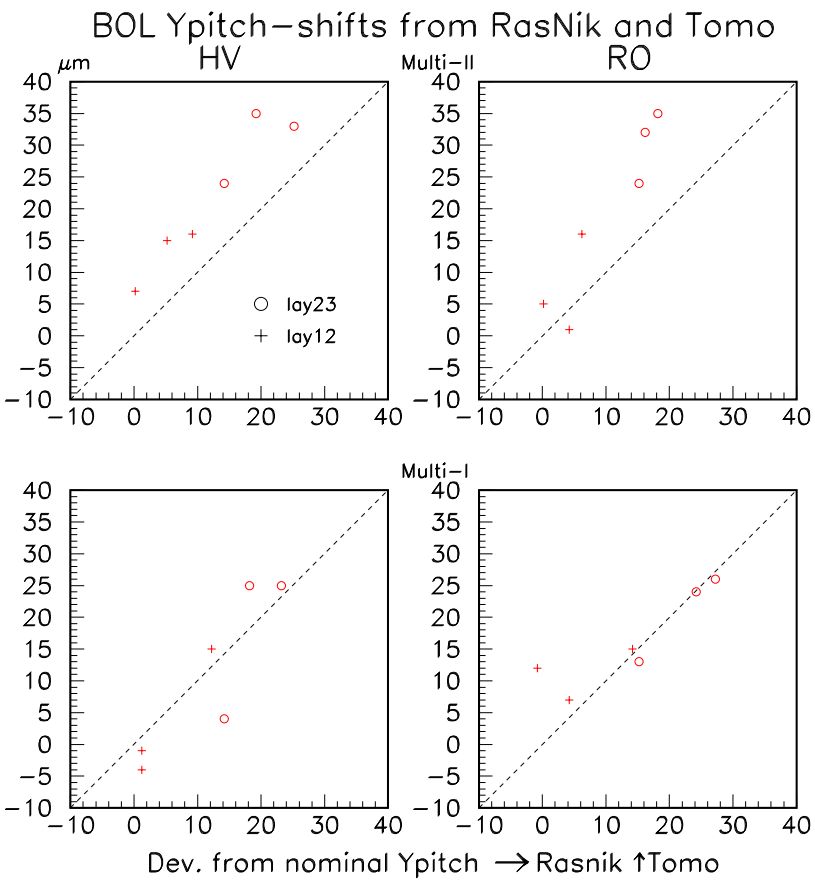

Figure 19: *tommie and ras y*

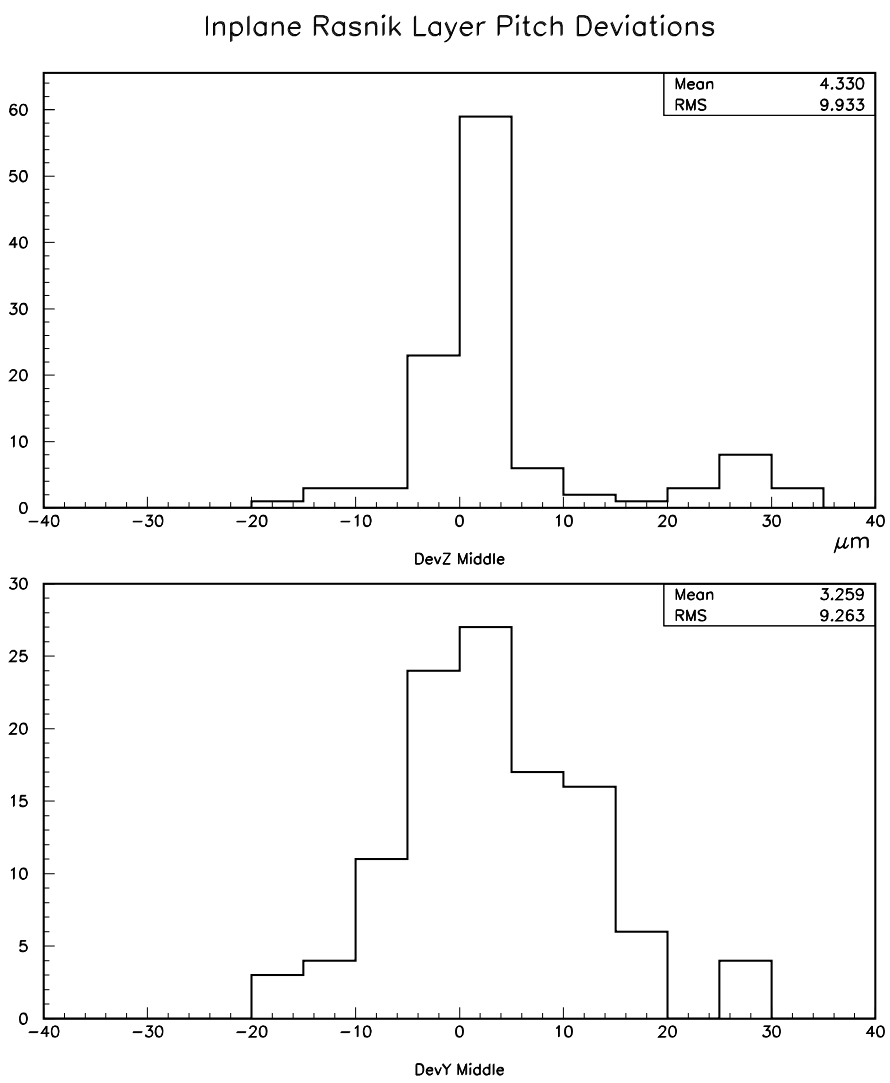

Figure 20: *his mid*

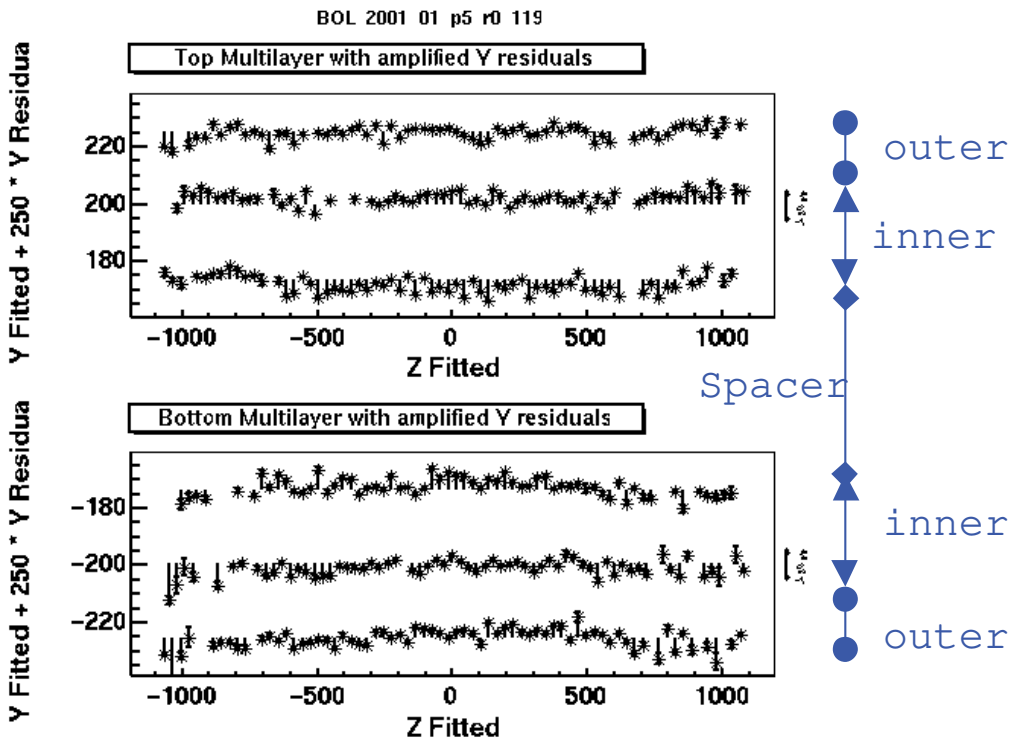

Figure 21: *Wire-map of BOL-0.*

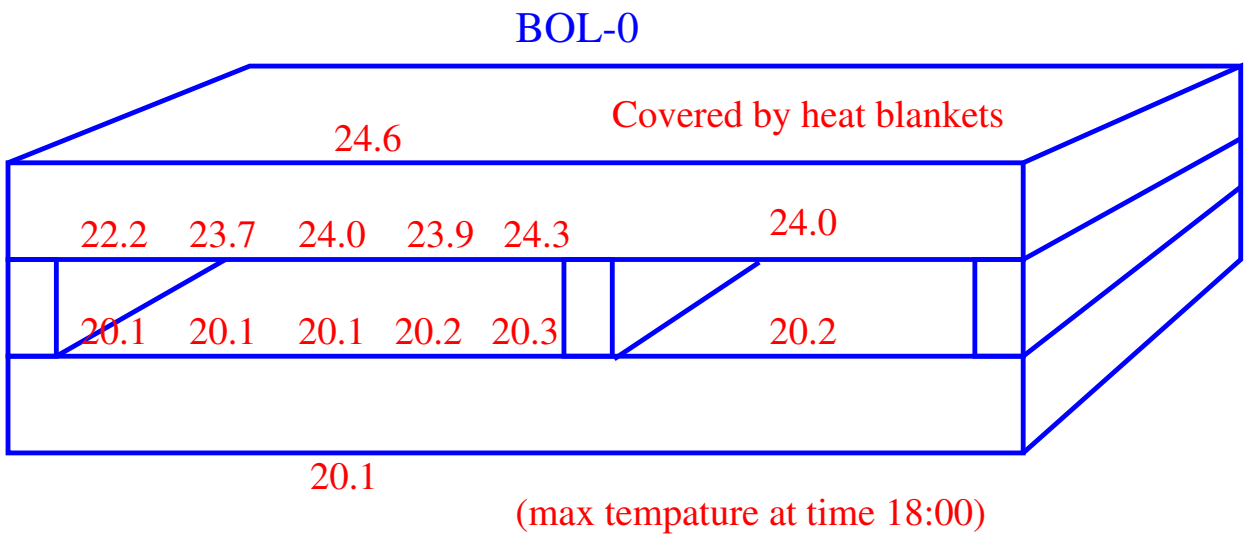

Figure 22: *Schematic view of the BOL0 chamber. The readings of the temperature sensors are indicated.*

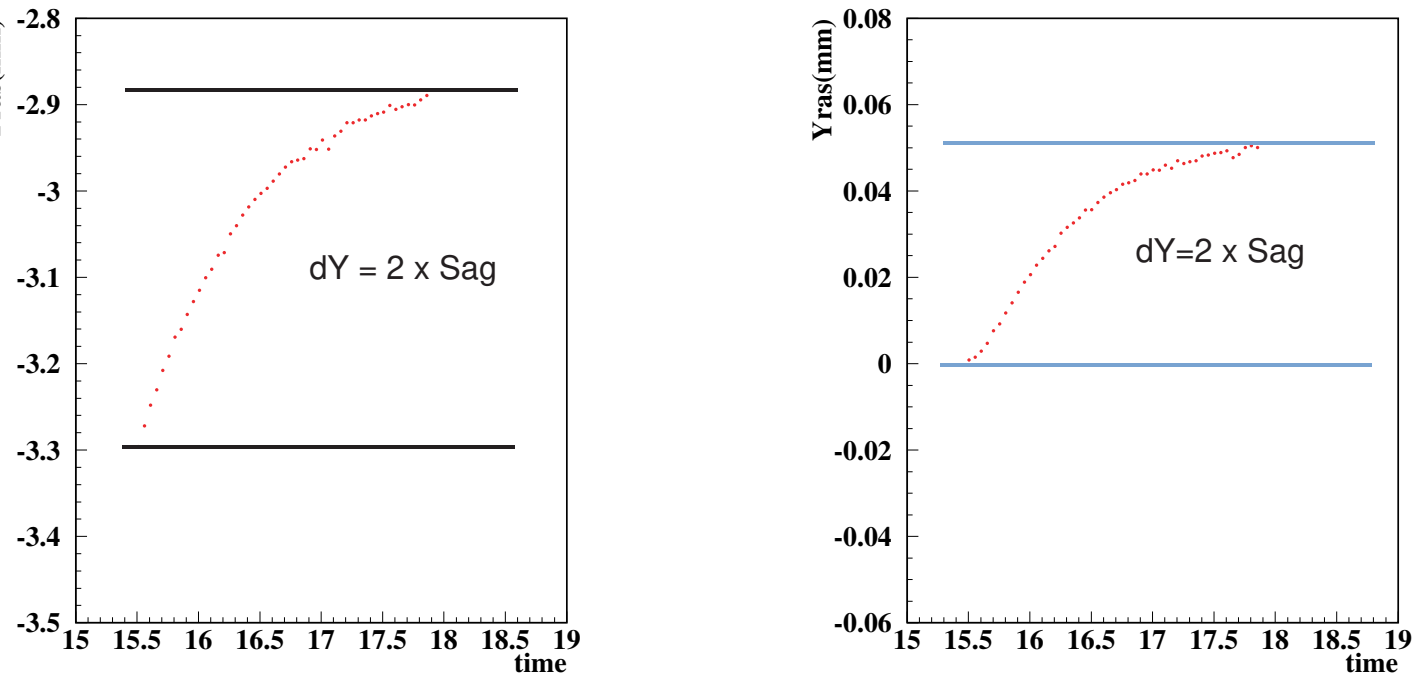

Figure 23: *a) Average Y of the in-plane system during heating, which is a measure of the chamber sag $\times$ 2. b) Measurement (Y) of a cross-plate RASNIK system , which is a measure of the cross-plate sag $\times$ 2.*

Distance CCD and Lens is 26mm nominal. However the supports should allow 10 mm displacements.

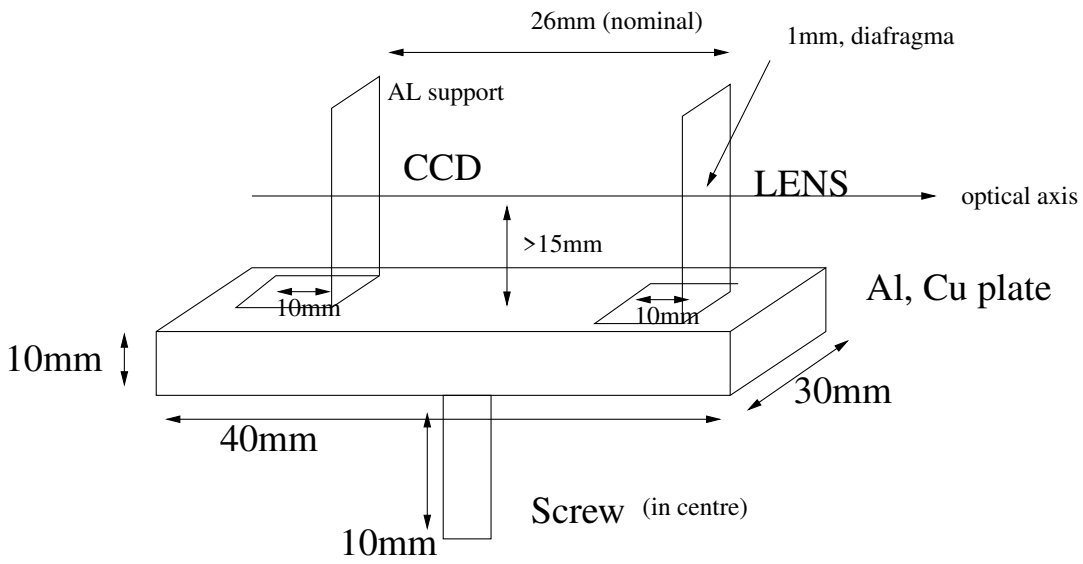

Figure 24: *Schematic view of the platform holding a CCD and lense. The platform can be mounted o n the 3D measuring device to calibrate the mask in calibration tower.*

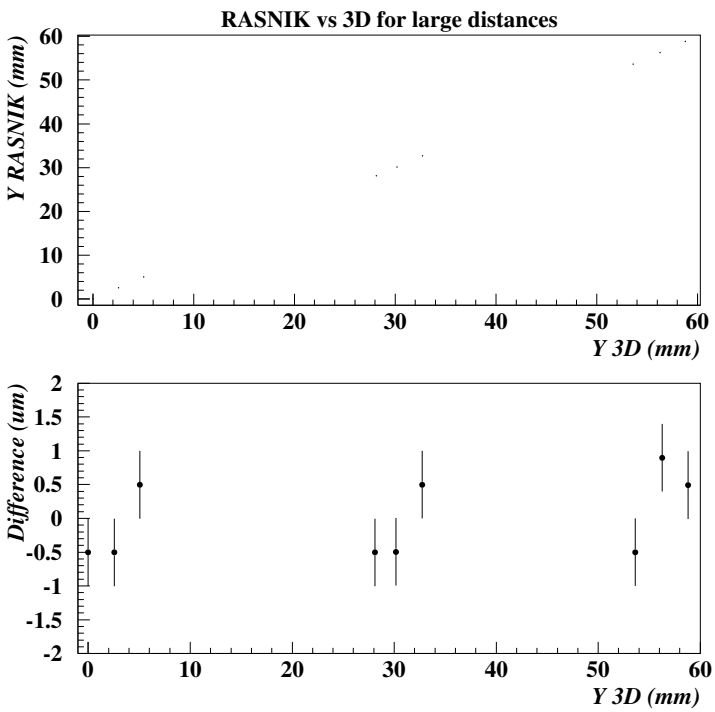

Figure 25: *top) Y-RASNIK versus Y-3D measurment device. bottom) The difference of RASNIK and the 3D device as function Y-3D.*

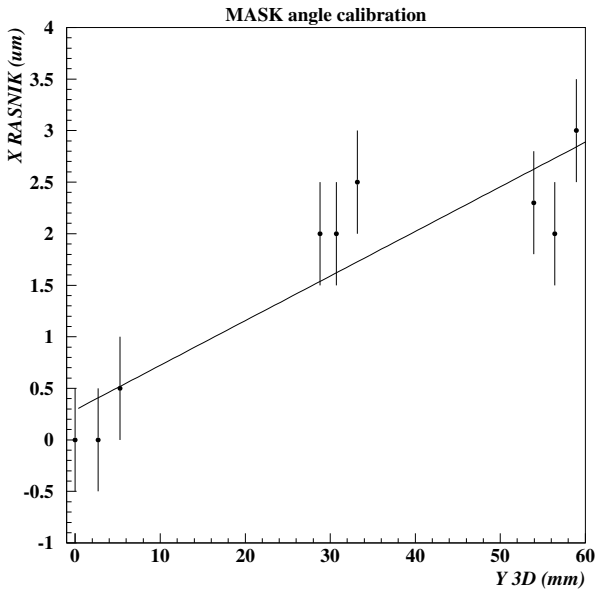

Figure 26: *The variation in RASNIK X as function Y of the 3D device. The fitted line is used to determine the rotation of the mask.*